


FIG. 1

GUIDEWIRE CHANNEL TO  
TOP POSITION

FIG. 2

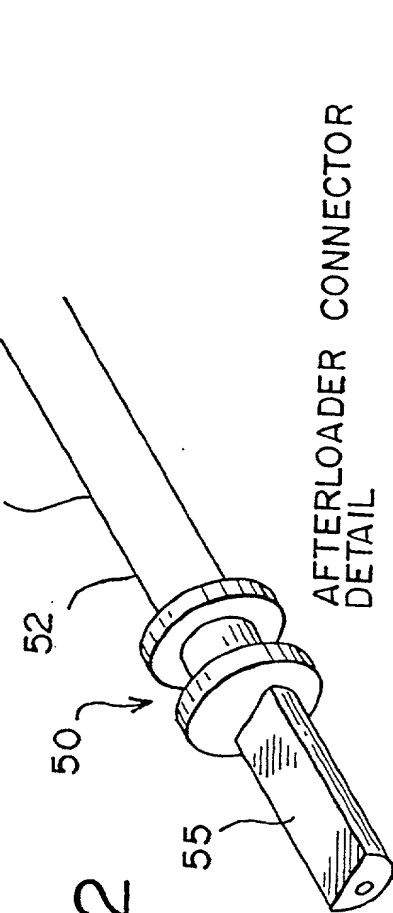


KEY TO PREVENT  
GUIDEWIRE ROTATION

GUIDEWIRE  
EXIT

GUIDEWIRE LUMEN  
ON TOP

GUIDEWIRE




55

52

12

52

FIG. 3

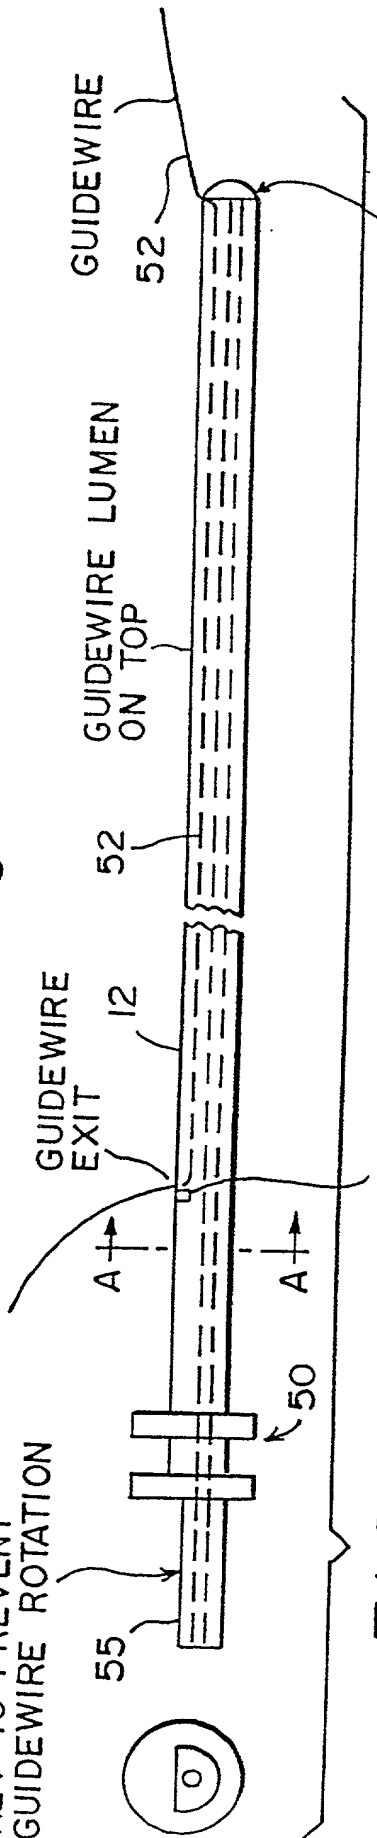

PLUG BEHIND EXIT  
TO STOP BLOOD  
FLOW TO  
AFTERLOADER


SEALED END  
RADIOTHERAPY  
CHANNEL.  
RADIO-OPAQUE  
TIP.

GUIDEWIRE  
LUMEN

SOURCE WIRE  
LUMEN

SECTION A-A

FIG. 3A

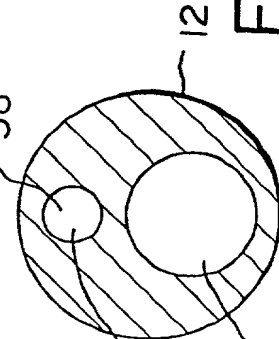

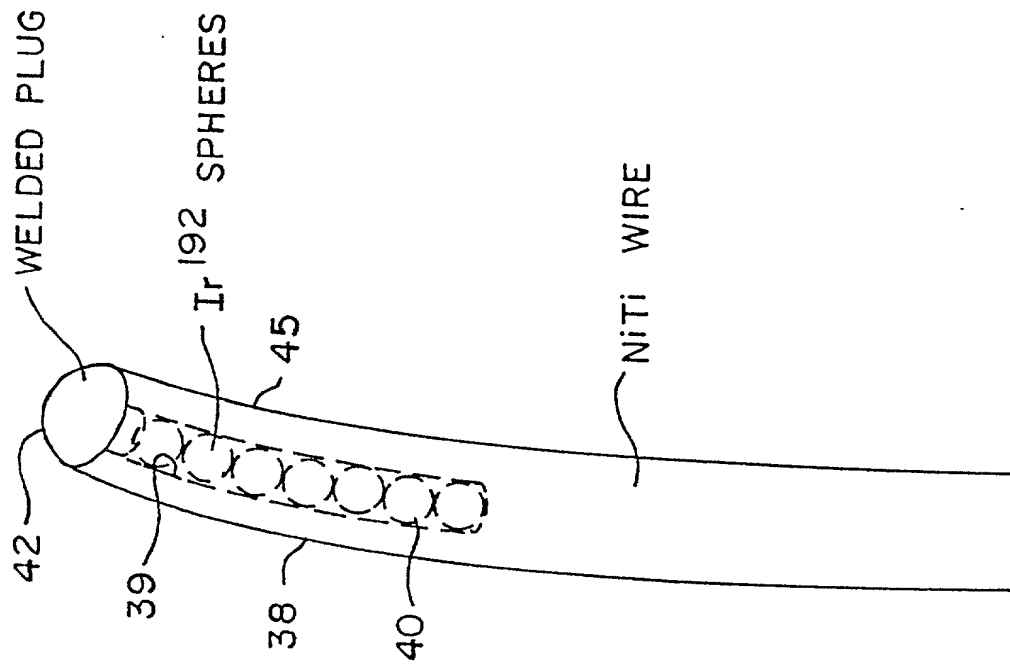


FIG. 4